

ZytoLight® SPEC SS18 Dual Color Break Apart Probe



Background


The ZytoLight® SPEC SS18 Dual Color Break Apart Probe (PL56) is intended to be used for the qualitative detection of translocations involving the human SS18 gene at 18q11.2 in formalin-fixed, paraffin-embedded specimens, such as synovial sarcoma, by fluorescence *in situ* hybridization (FISH). The probe is intended to be used in combination with the ZytoLight® FISH-Tissue Implementation Kit (Prod. No. Z-2028-5/-20).

The product is intended for professional use only. All tests using the product should be performed in a certified, licensed anatomic pathology laboratory under the supervision of a pathologist/human geneticist by qualified personnel. The probe is intended to be used as an aid to the differential diagnosis of synovial sarcoma and therapeutic measures should not be initiated based on the test result alone.


Probe Description

The ZytoLight® SPEC SS18 Dual Color Break Apart Probe is composed of:

- ZyGreen (excitation 503 nm/emission 528 nm) labeled polynucleotides (~10 ng/µl), which target sequences mapping in 18q11.2** (chr18:23,109,942-23,466,217) proximal to the SS18 breakpoint region.
- ZyOrange (excitation 547 nm/emission 572 nm) labeled polynucleotides (~4.5 ng/µl), which target sequences mapping in 18q11.2** (chr18:23,772,255-24,137,169) distal to the SS18 breakpoint region.
- Formamide based hybridization buffer

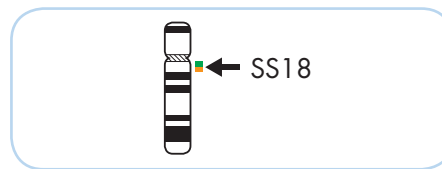


Ideogram of chromosome 18 indicating the hybridization locations.

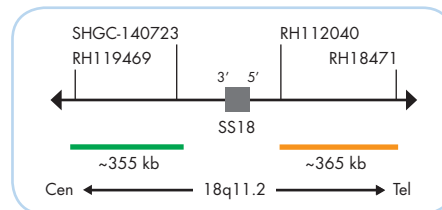


SPEC SS18 Probe map (not to scale).

Results

In an interphase nucleus lacking a translocation involving the 18q11.2 band two orange/green fusion signals are expected representing two normal (non-rearranged) 18q11.2 loci. A signal pattern consisting of one orange/green fusion signal, one orange signal, and a separate green signal indicates one normal 18q11.2 locus and one 18q11.2 locus affected by an 18q11.2 translocation.

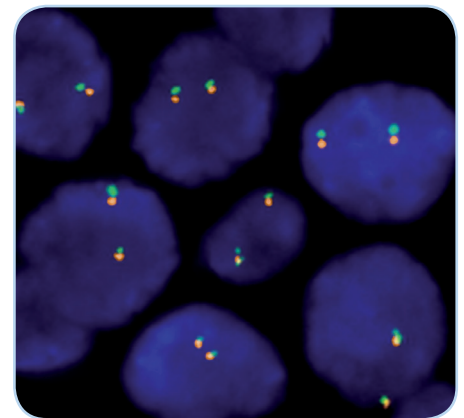

SPEC SS18 Dual Color Break Apart Probe hybridized to normal interphase cells as indicated by two orange/green fusion signals per nucleus.

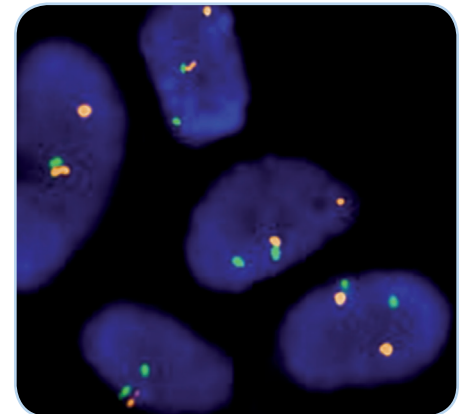

Synovial sarcoma tissue section with translocation affecting the 18q11.2 locus as indicated by one non-rearranged orange/green fusion signal, one orange signal, and one separate green signal.

| Prod. No. | Product | Label | Tests* (Volume) |
|------------------|---|-------|-----------------|
| Z-2097-50 | ZytoLight SPEC SS18 Dual Color Break Apart Probe CE IVD | ●/● | 5 (50 µl) |
| Z-2097-200 | ZytoLight SPEC SS18 Dual Color Break Apart Probe CE IVD | ●/● | 20 (200 µl) |
| Related Products | | | |
| Z-2028-5 | ZytoLight FISH-Tissue Implementation Kit CE IVD Incl. Heat Pretreatment Solution Citric, 150 ml; Pepsin Solution, 1 ml; Wash Buffer SSC, 210 ml; 25x Wash Buffer A, 50 ml; DAPI/DuraTect-Solution, 0.2 ml | | 5 |
| Z-2028-20 | ZytoLight FISH-Tissue Implementation Kit CE IVD Incl. Heat Pretreatment Solution Citric, 500 ml; Pepsin Solution, 4 ml; Wash Buffer SSC, 560 ml; 25x Wash Buffer A, 100 ml; DAPI/DuraTect-Solution, 0.8 ml | | 20 |

* Using 10 µl probe solution per test. IVD labeled products are only available in certain countries. All other countries research use only! Please contact your local dealer for more information.

**According to Human Genome Assembly GRCh37/hg19